

This manual contains instructions for the communication functions of the AER-102-PH.

To prevent accidents arising from the misuse of this instrument, please ensure the operator receives this manual.


Warning

Turn the power supply to the instrument off before wiring or checking.
Working on or touching the terminal with the power switched on may result in severe injury or death due to electrical shock.

1. System Configuration


System configuration example using Communication converter IF-400 and USB communication cable CMC-001-1

When using Communication converter IF-400

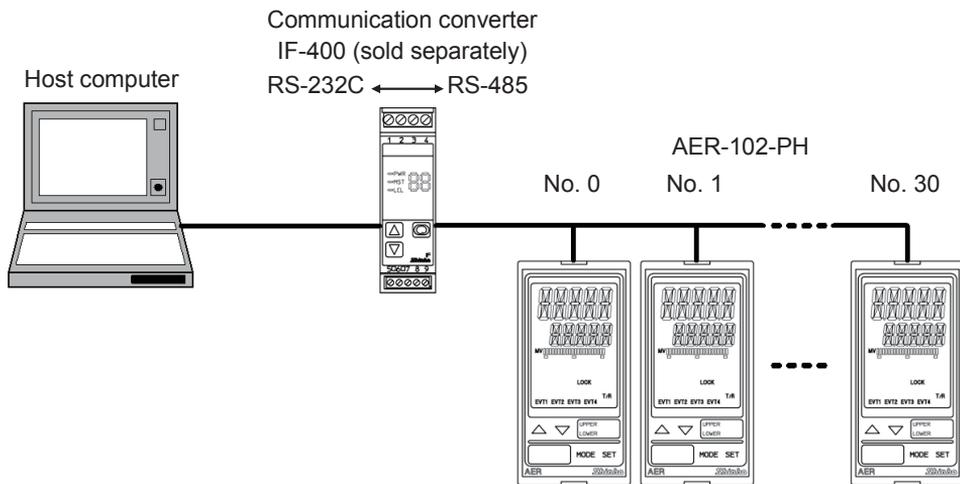

(Fig. 1-1)

When using USB communication cable CMC-001-1

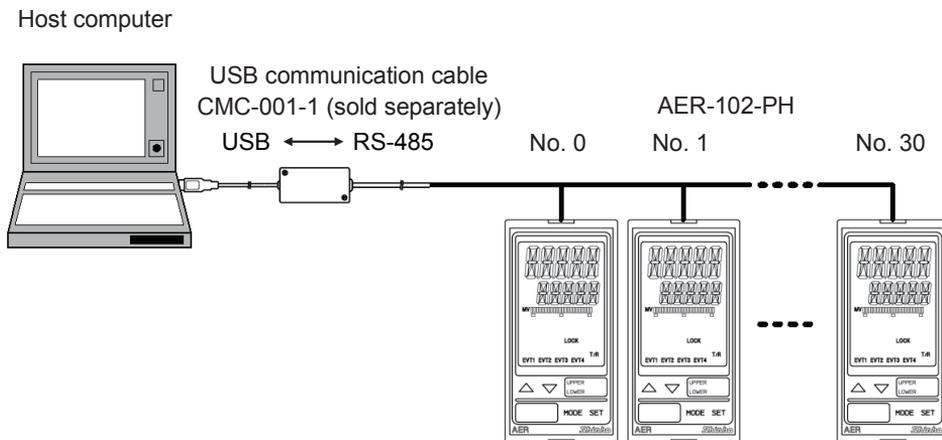

(Fig. 1-2)

2. Wiring

Wiring example using Communication converter IF-400 and USB communication cable CMC-001-1


When using Communication converter IF-400:

Use the included wire harness (C0J: Between IF-400 and AER-102-PH, C5J: Between AER-102-PH units), shield wire and CDM (sold separately).

When using USB Communication cable CMC-001-1:

Use the included wire harness (C0J: Between IF-400 and AER-102-PH, C5J: Between AER-102-PH units).

- When using Communication converter IF-400
- When using USB Communication cable CMC-001-1

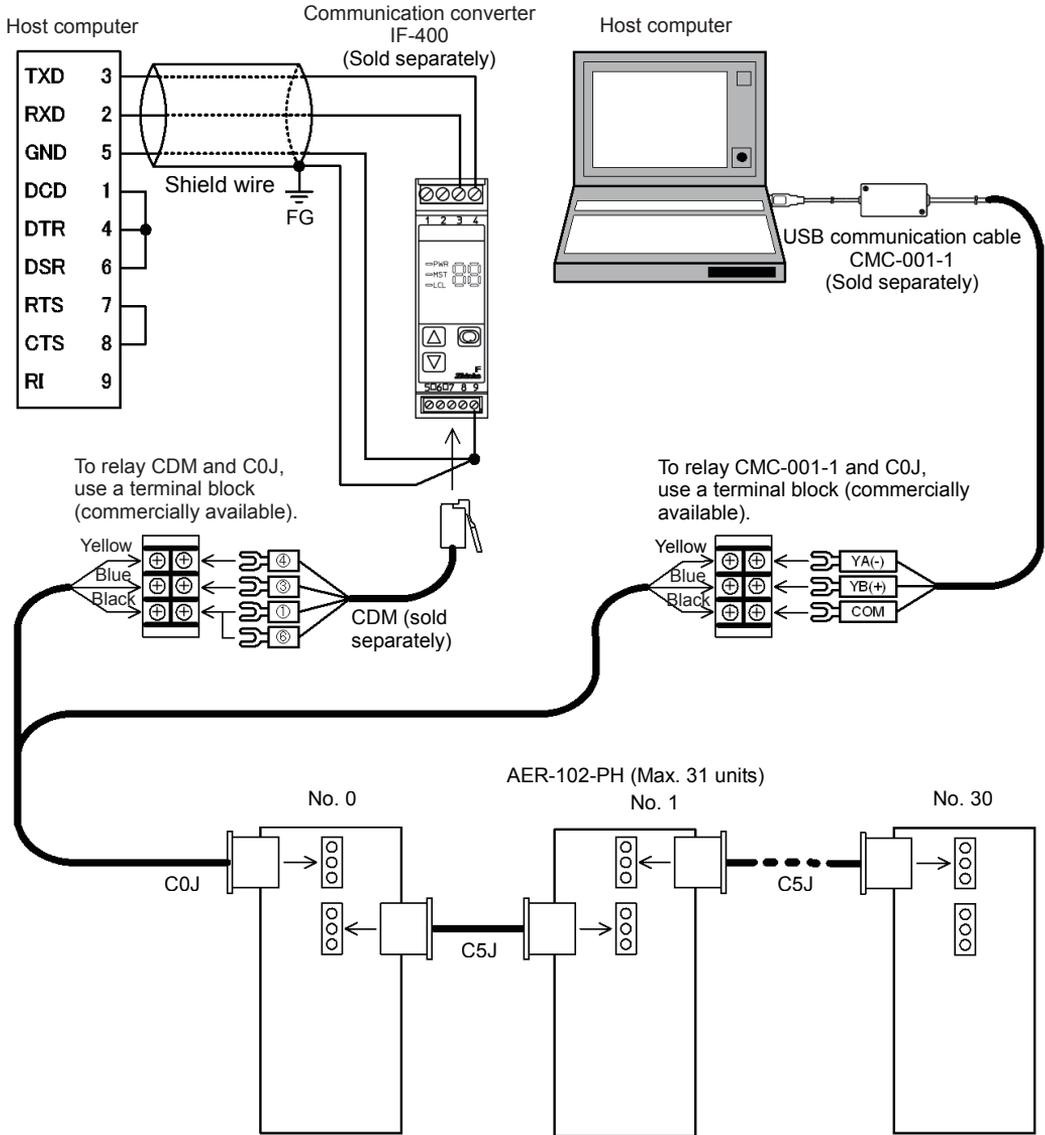

(Fig. 2-1)

Shield Wire

Connect only one end of the shield to the FG or GND terminal to avoid a ground loop. If both ends of the shield wire are connected to the FG or GND terminal, the circuit will be closed, resulting in a ground loop. This may cause noise. **Be sure to ground the FG or GND terminal.**

Recommended cable: OTSC-VB 2PX0.5SQ (made by Onamba Co., Ltd.) or equivalent (Use a twisted pair cable.)

Terminator (Terminal Resistor)

Communication converter IF-400 (sold separately) has a built-in terminator.

The terminator is mounted at the end of the wire when connecting multiple peripheral devices to a personal computer. The terminator prevents signal reflection and disturbance.

Do not connect a terminator to the communication line because each AER-102-PH has built-in pull-up and pull-down resistors.

3. Setting Communication Parameters

Communication parameters can be set in the Basic Function group.

To enter the Basic Function group, follow the procedure below.


- (1) \overline{cMFR} Press the **MODE** key 5 times in pH/Temperature Display Mode, or Cleansing Output Mode.
If EVT3, EVT4 Outputs (EVT3 option) are/is ordered, press the **MODE** key 7 times in pH/Temperature Display Mode, or Cleansing Output Mode.
- (2) \overline{cMHL} Press the **SET** key twice.
The unit enters the Basic Function group. "Communication protocol" item appears.
- (3) Make a selection using the Δ or ∇ key, and register the value by pressing the **SET** key.

Character	Setting Item, Function, Setting Range	Factory Default
\overline{cMHL} \overline{NoML}	Communication protocol <ul style="list-style-type: none"> • Selects communication protocol. • \overline{NoML} : Shinko protocol • \overline{ModR} : MODBUS ASCII mode • \overline{ModR} : MODBUS RTU mode 	Shinko protocol
\overline{cMNo} $\overline{0000}$	Instrument number <ul style="list-style-type: none"> • Sets the instrument number of this unit. (The instrument numbers should be set one by one when multiple instruments are connected in Serial communication, otherwise communication is not possible.) • Setting range: 0 to 95 	0
\overline{cMFR} $\overline{0096}$	Communication speed <ul style="list-style-type: none"> • Selects a communication speed equal to that of the host computer. • $\overline{0096}$: 9600 bps • $\overline{0092}$: 19200 bps • $\overline{00384}$: 38400 bps 	9600 bps
\overline{cMFR} $\overline{7EVEN}$	Data bit/Parity <ul style="list-style-type: none"> • Selects data bit and parity. • $\overline{8NoN}$: 8 bits/No parity • $\overline{7NoN}$: 7 bits/No parity • $\overline{8EVEN}$: 8 bits/Even • $\overline{7EVEN}$: 7 bits/Even • $\overline{8odd}$: 8 bits/Odd • $\overline{7odd}$: 7 bits/Odd 	7 bits/Even
\overline{cMFR} $\overline{0001}$	Stop bit <ul style="list-style-type: none"> • Selects the stop bit. • $\overline{0001}$: 1 bit • $\overline{0002}$: 2 bits 	1 bit

- (4) Press the **SET** key multiple times. The unit will revert to pH/Temperature Display Mode, or Cleansing Output Mode.

4. Communication Procedure

Communication starts with command transmission from the host computer (hereafter Master), and ends with the response of the AER-102-PH (hereafter Slave).

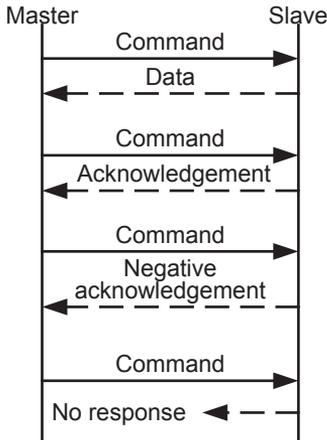

(Fig. 4-1)

- **Response with data**

When the master sends the reading command, the slave responds with the corresponding set value or current status.

- **Acknowledgement**

When the master sends the setting command, the slave responds by sending acknowledgement after the processing is terminated.

- **Negative acknowledgement**

When the master sends a non-existent command or value out of the setting range, the slave returns a negative acknowledgement.

- **No response**

The slave will not respond to the master in the following cases:

- Global address (Shinko protocol) is set.
- Broadcast address (MODBUS protocol) is set.
- Communication error (framing error, parity error)
- Checksum error (Shinko protocol), LRC discrepancy (MODBUS ASCII mode), CRC-16 discrepancy (MODBUS RTU mode)

Communication Timing of the RS-485

Master Side (Take note while programming)

When the master starts transmission through the RS-485 communication line, the master is arranged so as to provide an idle status (mark status) transmission period of 1 or more characters before sending the command to ensure synchronization on the receiving side.

Set the program so that the master can disconnect the transmitter from the communication line within a 1 character transmission period after sending the command in preparation for reception of the response from the slave.

To avoid collision of transmissions between the master and the slave, send the next command after carefully checking that the master has received the response.

If a response to the command is not returned due to communication errors, set the Retry Processing to send the command again. (It is recommended to execute Retry twice or more.)

Slave Side

When the slave starts transmission through the RS-485 communication line, the slave is arranged so as to provide an idle status (mark status) transmission period of 1 or more characters before sending the response to ensure synchronization on the receiving side.

The slave is arranged so as to disconnect the transmitter from the communication line within a 1 character transmission period after sending the response.

5. Shinko Protocol

5.1 Transmission Mode

Shinko protocol is composed of ASCII codes.

Hexadecimal (0 to 9, A to F), which is divided into high order (4-bit) and low order (4-bit) out of 8-bit binary data in command is transmitted as ASCII characters.

Data format Start bit: 1 bit
 Data bit: 7 bits
 Parity: Even
 Stop bit: 1 bit

Error detection: Checksum

5.2 Command Configuration

All commands are composed of ASCII.

The data (set value, decimal number) is represented by hexadecimal numbers.

Negative numbers are represented in 2's complement.

Numerals written below the command represent number of characters.

(1) Setting Command

Header (02H)	Address	Sub address (20H)	Command type (50H)	Data item	Data	Checksum	Delimiter (03H)
1	1	1	1	4	4	2	1

(2) Reading Command

Header (02H)	Address	Sub address (20H)	Command type (20H)	Data item	Checksum	Delimiter (03H)
1	1	1	1	4	2	1

(3) Response with Data

Header (06H)	Address	Sub address (20H)	Command type (20H)	Data item	Data	Checksum	Delimiter (03H)
1	1	1	1	4	4	2	1

(4) Acknowledgement

Header (06H)	Address	Checksum	Delimiter (03H)
1	1	2	1

(5) Negative Acknowledgement

Header (15H)	Address	Error code	Checksum	Delimiter (03H)
1	1	1	2	1

Header: Control code to represent the beginning of the command or the response. ASCII codes are used.

Setting command, Reading command: STX (02H) fixed

Response with data, Acknowledgement: ACK (06H) fixed

Negative acknowledgement: NAK (15H) fixed

Instrument number (Address): Numbers by which the master discerns each slave.

Instrument numbers 0 to 94 and Global address 95.

ASCII codes (20H to 7FH) are used by adding 20H to instrument numbers 0 to 95 (00H to 5FH).

95 (7FH) is called the Global address, which is used when the same command is sent to all the slaves connected. However, a response is not returned.

Sub address: 20H fixed

Command type: Code to discern Setting command (50H) and Reading command (20H)

- Data item:** Classification of the command object.
Composed of 4-digit hexadecimal numbers, using ASCII.
Refer to "7. Communication Command Table". (pp.11 to 21)
- Data:** The contents of data (set value) differ depending on the setting command.
Composed of 4-digit hexadecimal numbers, using ASCII.
Refer to "7. Communication Command Table". (pp. 11 to 21)
- Checksum:** 2-character data to detect communication errors. Refer to "5.3 Checksum Calculation".
- Delimiter:** Control code to represent the end of command.
ASCII code ETX (03H) fixed
- Error code:** Represents an error type using ASCII.
1 (31H)----Non-existent command
2 (32H)----Not used
3 (33H)----Setting outside the setting range
4 (34H)----Status unable to be set (e.g. During automatic calibration using the Automatic electrode quality evaluation function)
5 (35H)----During setting mode by keypad operation

5.3 Checksum Calculation

Checksum is used to detect receiving errors in the command or data.

Set the program for the master side as well to calculate the checksum of the response data from the slaves so that communication errors can be checked.

The ASCII code (hexadecimal) corresponding to the characters which range from the address (instrument number) to that before the checksum is converted to binary notation, and the total value is calculated.

The lower one byte of the total value is converted to 2's complement, and then to hexadecimal numbers, that is, ASCII code for the checksum.


Checksum Calculation Example

Data item 0008H (pH calibration value): 1.00 (0064H)

Address (instrument number): 0 (20H)

- 1's complement: Reverse each binary bit. 0 will become 1 and vice versa.
- 2's complement: Add 1 to 1's complement.

(e.g.)

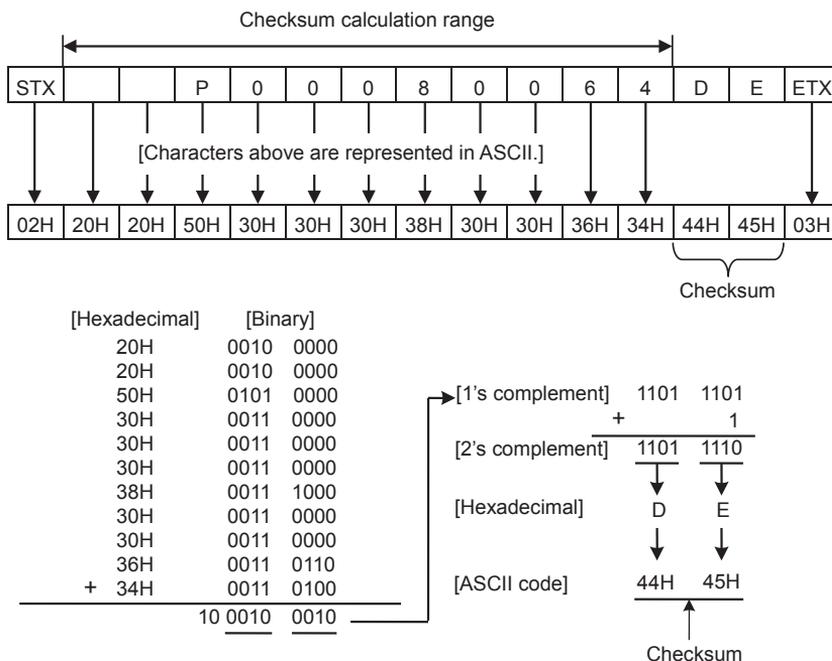

(Fig. 5.3-1)

6. MODBUS Protocol

6.1 Transmission Mode

There are 2 transmission modes (ASCII and RTU) in MODBUS protocol.

ASCII Mode

Hexadecimal (0 to 9, A to F), which is divided into high order (4-bit) and low order (4-bit) out of 8-bit binary data in command is transmitted as ASCII characters.

Data format Start bit: 1 bit
 Data bit: 7 bits (8 bits) (Selectable)
 Parity: Even (No parity, Odd) (Selectable)
 Stop bit: 1 bit (2 bits) (Selectable)
 Error detection : LRC (Longitudinal Redundancy Check)

RTU Mode

8-bit binary data in command is transmitted as it is.

Data format Start bit: 1 bit
 Data bit: 8 bits
 Parity: No parity (Even, Odd) (Selectable)
 Stop bit: 1 bit (2 bits) (Selectable)
 Error detection: CRC-16 (Cyclic Redundancy Check)

6.2 Data Communication Interval

ASCII Mode

Max.1 second of interval between ASCII mode characters

RTU Mode

Communication speed 9600 bps, 19200 bps:

To transmit continuously, an interval between characters which consist of one message, must be within 1.5-character transmission times.

Communication speed 38400 bps:

To transmit continuously, an interval between characters which consist of one message, must be within 750 μ s.

If an interval lasts longer than 1.5-character transmission times or 750 μ s, the AER-102-PH assumes that transmission from the master is finished, which results in a communication error, and will not return a response.

6.3 Message Configuration

ASCII Mode

ASCII mode message is configured to start by Header [: (colon) (3AH)] and end by Delimiter [CR (carriage return) (0DH) + LF (Line feed) (0AH)].

Header (:)	Slave address	Function code	Data	Error check LRC	Delimiter (CR)	Delimiter (LF)
---------------	------------------	------------------	------	--------------------	-------------------	-------------------

RTU Mode

Communication speed 9600 bps, 19200 bps: RTU mode is configured to start after idle time is processed for more than 3.5-character transmissions, and end after idle time is processed for more than 3.5-character transmissions.

Communication speed 38400 bps: RTU mode is configured to start after idle time is processed for more than 1.75 ms, and end after idle time is processed for more than 1.75 ms.

3.5 idle characters	Slave address	Function code	Data	Error check CRC-16	3.5 idle characters
------------------------	------------------	------------------	------	-----------------------	------------------------

6.3.1 Slave Address

Slave address is an individual instrument number on the slave side, and is set within the range 0 to 95 (00H to 5FH). The master identifies slaves by the slave address of the requested message. The slave informs the master which slave is responding to the master by placing its own address in the response message.

Slave address 00H (Broadcast address) can identify all the slaves connected. However, slaves do not respond.

6.3.2 Function Code

The function code is the command code for the slave to undertake one of the following actions.

(Table 6.3.2-1)

Function Code	Contents
03 (03H)	Reading the set value and information from slaves
06 (06H)	Setting to slaves

The Function code is used to discern whether the response is normal (acknowledgement) or if any error (negative acknowledgement) has occurred when the slave returns the response message to the master.

When acknowledgement is returned, the slave simply returns the original function code.

When negative acknowledgement is returned, the MSB of the original function code is set as 1 for the response.

(For example, if the master sends request message setting 10H to the function code by mistake, slave returns 90H by setting the MSB to 1, because the former is an illegal function.)

For negative acknowledgement, the exception codes below are set to the data of the response message, and returned to the master in order to inform it of what kind of error has occurred.

(Table 6.3.2-2)

Exception Code	Contents
1 (01H)	Illegal function (Non-existent function)
2 (02H)	Illegal data address (Non-existent data address)
3 (03H)	Illegal data value (Value out of the setting range)
17 (11H)	Shinko protocol error code 4 (Status unable to be set) (e.g.) During automatic calibration using the Automatic electrode quality evaluation function
18 (12H)	Shinko protocol error code 5 (During setting mode by keypad operation)

6.3.3 Data

Data differs depending on the function code.

A request message from the master is composed of a data item, amount of data and setting data.

A response message from the slave is composed of the byte count, data and exception codes in negative acknowledgements.

The effective range of data is -32768 to 32767 (8000H to 7FFFH).

6.3.4 Error Check

ASCII Mode

After calculating LRC (Longitudinal Redundancy Check) from the slave address to the end of data, the calculated 8-bit data is converted to two ASCII characters, and are appended to the end of message.

How to calculate LRC

- ① Create a message in RTU mode.
- ② Add all the values from the slave address to the end of data. This is assumed as X.
- ③ Make a complement for X (bit reverse). This is assumed as X.
- ④ Add a value of 1 to X. This is assumed as X.
- ⑤ Set X as an LRC to the end of the message.
- ⑥ Convert the whole message to ASCII characters.

RTU Mode

After calculating CRC-16 (Cyclic Redundancy Check) from the slave address to the end of the data, the calculated 16-bit data is appended to the end of message in sequence from low order to high order.

How to calculate CRC-16

In the CRC-16 system, the information is divided by the polynomial series. The remainder is added to the end of the information and transmitted. The generation of a polynomial series is as follows.

(Generation of polynomial series: $X^{16} + X^{15} + X^2 + 1$)

- ① Initialize the CRC-16 data (assumed as X) (FFFFH).
- ② Calculate exclusive OR (XOR) with the 1st data and X. This is assumed as X.
- ③ Shift X one bit to the right. This is assumed as X.

- ④ When a carry is generated as a result of the shift, XOR is calculated by X of ③ and the fixed value (A001H). This is assumed as X. If a carry is not generated, go to step ⑤.
- ⑤ Repeat steps ③ and ④ until shifting 8 times.
- ⑥ XOR is calculated with the next data and X. This is assumed as X.
- ⑦ Repeat steps ③ to ⑤.
- ⑧ Repeat steps ③ to ⑤ up to the final data.
- ⑨ Set X as CRC-16 to the end of message in sequence from low order to high order.

6.4 Message Example

ASCII Mode

Numerals written below the command represent the number of characters.

① Reading [Slave address 1, Data item 0080H (pH)]

- A request message from the master

Amount of data means how many data items are to be read. It is fixed as (30H 30H 30H 31H).

Header	Slave address	Function code	Data item [0080H]	Amount of data [0001H]	Error check LRC	Delimiter
(3AH)	(30H 31H)	(30H 33H)	(30H 30H 38H 30H)	(30H 30H 30H 31H)	(37H 42H)	(0DH 0AH)
1	2	2	4	4	2	2

- Response message from the slave in normal status [(e.g.) pH 1.00 (0064H)]

The response byte count means the byte count of data which have been read.

It is fixed as (30H 32H).

Header	Slave address	Function code	Response byte count [02H]	Data [0064H]	Error check LRC	Delimiter
(3AH)	(30H 31H)	(30H 33H)	(30H 32H)	(30H 30H 36H 34H)	(39H 36H)	(0DH 0AH)
1	2	2	2	4	2	2

- Response message from the slave in exception (error) status (When a data item is incorrect)
The function code MSB is set to 1 for the response message in exception (error) status (83H is returned). The exception code 02H (Non-existent data address) is returned (error).

Header	Slave address	Function code	Exception code [02H]	Error check LRC	Delimiter
(3AH)	(30H 31H)	(38H 33H)	(30H 32H)	(37H 41H)	(0DH 0AH)
1	2	2	2	2	2

② Setting [Slave address 1, Data item 0008H (pH calibration value)]

- A request message from the master [When pH calibration value is set to 1.00 (0064H)]

Header	Slave address	Function code	Data item [0008H]	Data [0064H]	Error check LRC	Delimiter
(3AH)	(30H 31H)	(30H 36H)	(30H 30H 30H 38H)	(30H 30H 36H 34H)	(38H 44H)	(0DH 0AH)
1	2	2	4	4	2	2

- Response message from the slave in normal status

Header	Slave address	Function code	Data item [0008H]	Data [0064H]	Error check LRC	Delimiter
(3AH)	(30H 31H)	(30H 36H)	(30H 30H 30H 38H)	(30H 30H 36H 34H)	(38H 44H)	(0DH 0AH)
1	2	2	4	4	2	2

- Response message from the slave in exception (error) status (When a value out of the setting range is set.)

The function code MSB is set to 1 for the response message in exception (error) status (86H is returned). The exception code 03H (Value out of the setting range) is returned (error).

Header	Slave address	Function code	Exception code [03H]	Error check LRC	Delimiter
(3AH)	(30H 31H)	(38H 36H)	(30H 33H)	(37H 36H)	(0DH 0AH)
1	2	2	2	2	2

RTU Mode

Numerals written below the command represent number of characters.

① Reading [Slave address 1, Data item 0080H (pH)]

- A request message from the master

Amount of data means how many data items are to be read. It is fixed as (0001H).

3.5 idle characters	Slave address (01H)	Function code (03H)	Data item (0080H)	Amount of data (0001H)	Error check CRC-16 (85E2H)	3.5 idle characters
	1	1	2	2	2	

- Response message from the slave in normal status [(e.g.) pH 1.00 (0064H)]

The response byte count means the byte count of data which has been read.

It is fixed as (02H).

3.5 idle characters	Slave address (01H)	Function code (03H)	Response byte count (02H)	Data (0064H)	Error check CRC-16 (B9AFH)	3.5 idle characters
	1	1	1	2	2	

- Response message from the slave in exception (error) status (When a data item is incorrect)

The function code MSB is set to 1 for the response message in exception (error) status (83H is returned).

The exception code (02H: Non-existent data address) is returned (error).

3.5 idle characters	Slave address (01H)	Function code (83H)	Exception code (02H)	Error check CRC-16 (C0F1H)	3.5 idle characters
	1	1	1	2	

② Setting (Slave address 1, Data item 0008H (pH calibration value))

- A request message from the master [When pH calibration value is set to 1.00 (0064H)]

3.5 idle characters	Slave address (01H)	Function code (06H)	Data item (0008H)	Data (0064H)	Error check CRC-16 (D9E3H)	3.5 idle characters
	1	1	2	2	2	

- Response message from the slave in normal status

3.5 idle characters	Slave address (01H)	Function code (06H)	Data item (0008H)	Data (0064H)	Error check CRC-16 (D9E3H)	3.5 idle characters
	1	1	2	2	2	

- Response message from the slave in exception (error) status (When a value out of the setting range is set)

The function code MSB is set to 1 for the response message in exception (error) status (86H is returned.).

The exception code (03H: Value out of the setting range) is returned (error).

3.5 idle characters	Slave address (01H)	Function code (86H)	Exception code (03H)	Error check CRC-16 (0261H)	3.5 idle characters
	1	1	1	2	

7. Communication Command Table

7.1 Notes about Setting/Reading Command

- The data (set value, decimal) is converted to hexadecimal numbers. Negative numbers are represented in 2's complement.
- When connecting multiple slaves, the address (instrument number) must not be duplicated.
- Data items 0200H to 0209H (User save area 1 to 10) can be read or set in 1 word units. Effective range of data is -32768 to 32767 (8000H to 7FFFH).
- MODBUS protocol uses Holding Register addresses. The Holding Register addresses are created as follows. A Shinko command data item is converted to decimal number, and the offset of 40001 is added. The result is the Holding Register address.
Using Data item 0001H (2nd solution) as an example: Data item in the sending message is 0001H, however, MODBUS protocol Holding Register address is 40002 (1 + 40001).
- Even if options are not ordered, setting or reading via software communication will be possible. However, EVT3, EVT4 and Transmission output 2 command contents will not function.

(1) Setting Command

- Up to 1,000,000 (one million) entries can be stored in non-volatile IC memory. If the number of settings exceeds the limit, the data will not be saved. So, do not change the set values frequently via software communication. (If a value set via software communication is the same as the value before the setting, the value will not be written in non-volatile IC memory.)
- Be sure to select Lock 3 when changing the set value frequently via software communication. If Lock 3 is selected, all set values – except Electrode RTD, Temperature calibration value, pH calibration value, pH calibration Auto/Manual, Transmission output 1 Zero and Span adjustment values, Transmission output 2 Zero and Span adjustment values – can be temporarily changed. However, they revert to their previous value after the power is turned off because they are not saved in the non-volatile IC memory. Do not change setting items such as EVT1, EVT2, EVT3 and EVT4 types. If they are changed, they will affect other setting items.
- Setting range of each item is the same as that of keypad operation.
- When the data (set value) has a decimal point, a whole number (hexadecimal) without a decimal point is used.
- If EVT1, EVT2, EVT3 or EVT4 type is changed at Data items 0003H (EVT1 type), 0050H (EVT2 type), 0051H (EVT3 type) or 0052H (EVT4 type), the EVT1, EVT2, EVT3 or EVT4 value will default to 0 (zero). The output status of EVT1, EVT2, EVT3 or EVT4 will also be initialized.
- Settings via software communication are possible while in Set value lock status.
- Communication parameters such as Instrument Number, Communication Speed of the slave cannot be set by software communication. They can only be set via the keypad.
- When sending a command by Global address [95 (7FH), Shinko protocol] or Broadcast address [(00H), MODBUS protocol], the same command is sent to all the slaves connected. However, the response is not returned.

(2) Reading Command

- When the data (set value) has a decimal point, a whole number (hexadecimal) without a decimal point is used for a response.

7.2 Setting/Reading Command

Shinko Command Type	MODBUS Function Code	Data Item		Data
50H/20H	06H/03H	0001H	2nd solution	0000H: pH 2 0001H: pH 4 0002H: pH 9 0003H: pH 10
50H/20H	06H/03H	0002H	pH input decimal point place	0000H: No decimal point 0001H: 1 digit after decimal point 0002H: 2 digits after decimal point
50H/20H	06H/03H	0003H	EVT1 type	0000H: No action 0001H: pH input low limit action 0002H: pH input high limit action 0003H: Temperature input low limit action 0004H: Temperature input high limit action 0005H: Error output 0006H: Fail output 0007H: Cleansing output 0008H: pH input error alarm output 0009H: pH fluctuation alarm output 000AH: pH input High/Low limits independent action 000BH: Temperature input High/Low limits independent action
50H/20H	06H/03H	0004H	EVT1 value	Set value (Decimal point ignored.)
50H/20H	06H/03H	0005H	EVT1 ON side	Set value (Decimal point ignored.)
50H/20H	06H/03H	0006H	EVT1 ON delay time	Set value
50H/20H	06H/03H	0007H	EVT1 OFF delay time	Set value
50H/20H	06H/03H	0008H	pH calibration value	Set value (Decimal point ignored.)
50H/20H	06H/03H	0009H	pH 7 calibration standard	0000H: JIS 0001H: US standard JIS stands for Japanese Industrial Standards.
50H/20H	06H/03H	0010H	EVT1 proportional band	Set value (Decimal point ignored.)
50H/20H	06H/03H	0011H	EVT1 reset	Set value (Decimal point ignored.)
50H/20H	06H/03H	0012H	EVT1 proportional cycle	Set value
50H/20H	06H/03H	0013H	EVT2 proportional band	Set value (Decimal point ignored.)
50H/20H	06H/03H	0014H	EVT2 reset	Set value (Decimal point ignored.)
50H/20H	06H/03H	0015H	EVT2 proportional cycle	Set value
50H/20H	06H/03H	0016H	EVT3 proportional band	Set value (Decimal point ignored.)
50H/20H	06H/03H	0017H	EVT3 reset	Set value (Decimal point ignored.)
50H/20H	06H/03H	0018H	EVT3 proportional cycle	Set value
50H/20H	06H/03H	0019H	EVT4 proportional band	Set value (Decimal point ignored.)
50H/20H	06H/03H	001AH	EVT4 reset	Set value (Decimal point ignored.)
50H/20H	06H/03H	001BH	EVT4 proportional cycle	Set value
50H/20H	06H/03H	0021H	Electrode RTD	Pt spec: 0000H: No temperature compensation 0001H: Pt1000 0002H: Pt100 Cu spec: 0000H: No temperature compensation 0001H: Cu500
50H/20H	06H/03H	0022H	Temperature input decimal point place	0000H: No decimal point 0001H: 1 digit after decimal point
50H/20H	06H/03H	0023H	Reference temperature	Set value (Decimal point ignored.)
50H/20H	06H/03H	0028H	Temperature calibration value	Set value (Decimal point ignored.)

Shinko Command Type	MODBUS Function Code	Data Item		Data
50H/20H	06H/03H	0030H	Set value lock	0000H: Unlock 0001H: Lock 1 0002H: Lock 2 0003H: Lock 3
50H/20H	06H/03H	0031H	Transmission output 1 type	0000H: pH transmission 0001H: Temperature transmission 0002H: MV1 transmission (*1) 0003H: MV2 transmission 0004H: MV3 transmission (*2) 0005H: MV4 transmission (*2)
50H/20H	06H/03H	0032H	Transmission output 1 high limit	Set value (Decimal point ignored.)
50H/20H	06H/03H	0033H	Transmission output 1 low limit	Set value (Decimal point ignored.)
50H/20H	06H/03H	0034H	pH calibration Auto/Manual	0000H: Automatic 0001H: Manual
50H/20H	06H/03H	0037H	Backlight time	Set value
50H	06H	0038H	pH calibration mode	0000H: pH/Temperature Display Mode, or Cleansing Output Mode 0001H: Calibration mode
50H	06H	0039H	pH calibration start	0001H: 1st point calibration start 0002H: 1st point calibration complete 0003H: 2nd point calibration start 0004H: 2nd point calibration complete
50H/20H	06H/03H	0040H	pH input filter time constant	Set value (Decimal point ignored.)
50H/20H	06H/03H	0041H	EVT output when input errors occur	0000H: Enabled 0001H: Disabled
50H/20H	06H/03H	0042H	Cable length correction	Set value (Decimal point ignored.)
50H/20H	06H/03H	0043H	Cable cross-section area	Set value (Decimal point ignored.)
50H/20H	06H/03H	0048H	Output ON time when EVT1 output ON	Set value
50H/20H	06H/03H	0049H	Output OFF time when EVT1 output ON	Set value
50H/20H	06H/03H	004AH	Output ON time when EVT2 output ON	Set value
50H/20H	06H/03H	004BH	Output OFF time when EVT2 output ON	Set value
50H/20H	06H/03H	004CH	Output ON time when EVT3 output ON	Set value
50H/20H	06H/03H	004DH	Output OFF time when EVT3 output ON	Set value
50H/20H	06H/03H	004EH	Output ON time when EVT4 output ON	Set value
50H/20H	06H/03H	004FH	Output OFF time when EVT4 output ON	Set value

(*1) If 'Setting' is executed while Transmission output 2 (TA2 option) is ordered, the following error code will be returned.

- Shinko protocol: Error code 3 (33H)
- MODBUS: Exception code 3 (03H)

(*2) If 'Setting' is executed while EVT3, EVT4 outputs (EVT3 option) are/is not ordered, the following error code will be returned.

- Shinko protocol: Error code 3 (33H)
- MODBUS: Exception code 3 (03H)

Shinko Command Type	MODBUS Function Code	Data Item		Data
50H/20H	06H/03H	0050H	EVT2 type	0000H: No action 0001H: pH input low limit action 0002H: pH input high limit action 0003H: Temperature input low limit action 0004H: Temperature input high limit action 0005H: Error output 0006H: Fail output 0007H: Cleansing output 0008H: pH input error alarm output 0009H: pH fluctuation alarm output 000AH: pH input High/Low limits independent action 000BH: Temperature input High/Low limits independent action
50H/20H	06H/03H	0051H	EVT3 type	0000H: No action 0001H: pH input low limit action 0002H: pH input high limit action 0003H: Temperature input low limit action 0004H: Temperature input high limit action 0005H: Error output 0006H: Fail output 0007H: Cleansing output 0008H: pH input error alarm output 0009H: pH fluctuation alarm output 000AH: pH input High/Low limits independent action 000BH: Temperature input High/Low limits independent action
50H/20H	06H/03H	0052H	EVT4 type	0000H: No action 0001H: pH input low limit action 0002H: pH input high limit action 0003H: Temperature input low limit action 0004H: Temperature input high limit action 0005H: Error output 0006H: Fail output 0007H: Cleansing output 0008H: pH input error alarm output 0009H: pH fluctuation alarm output 000AH: pH input High/Low limits independent action 000BH: Temperature input High/Low limits independent action
50H/20H	06H/03H	0053H	EVT2 value	Set value (Decimal point ignored.)
50H/20H	06H/03H	0054H	EVT3 value	Set value (Decimal point ignored.)
50H/20H	06H/03H	0055H	EVT4 value	Set value (Decimal point ignored.)
50H/20H	06H/03H	0056H	EVT2 ON side	Set value (Decimal point ignored.)
50H/20H	06H/03H	0057H	EVT3 ON side	Set value (Decimal point ignored.)
50H/20H	06H/03H	0058H	EVT4 ON side	Set value (Decimal point ignored.)
50H/20H	06H/03H	0059H	EVT2 ON delay time	Set value
50H/20H	06H/03H	005AH	EVT3 ON delay time	Set value
50H/20H	06H/03H	005BH	EVT4 ON delay time	Set value
50H/20H	06H/03H	005CH	EVT2 OFF delay time	Set value
50H/20H	06H/03H	005DH	EVT3 OFF delay time	Set value
50H/20H	06H/03H	005EH	EVT4 OFF delay time	Set value

Shinko Command Type	MODBUS Function Code	Data Item		Data
50H/20H	06H/03H	0063H	Backlight selection	0000H: All are backlit 0001H: pH Display 0002H: Temperature Display 0003H: Action indicators 0004H: pH Display + Temperature Display 0005H: pH Display + Action indicators 0006H: Temperature Display + Action indicators
50H/20H	06H/03H	0064H	pH color	0000H: Green 0001H: Red 0002H: Orange 0003H: pH color changes continuously
50H/20H	06H/03H	0065H	pH color range	Set value (Decimal point ignored.)
50H/20H	06H/03H	0066H	Bar graph indication	0000H: No indication 0001H: Transmission output 1 0002H: Transmission output 2 (*)
50H/20H	06H/03H	0067H	pH color reference value	Set value (Decimal point ignored.)
50H/20H	06H/03H	0068H	pH input sensor correction	Set value (Decimal point ignored.)
50H/20H	06H/03H	0069H	Temperature Display when no temperature compensation	0000H: Unlit 0001H: Reference temperature
50H/20H	06H/03H	006FH	Pt100 input wire type	0000H: 2-wire type 0001H: 3-wire type
50H/20H	06H/03H	0070H	EVT1 output high limit	Set value
50H/20H	06H/03H	0071H	EVT1 output low limit	Set value
50H/20H	06H/03H	0072H	EVT2 output high limit	Set value
50H/20H	06H/03H	0073H	EVT2 output low limit	Set value
50H/20H	06H/03H	0074H	EVT3 output high limit	Set value
50H/20H	06H/03H	0075H	EVT3 output low limit	Set value
50H/20H	06H/03H	0076H	EVT4 output high limit	Set value
50H/20H	06H/03H	0077H	EVT4 output low limit	Set value
50H	06H	007FH	Key operation change flag clearing	0001H: Clear change flag
50H/20H	06H/03H	0100H	EVT1 hysteresis type	0000H: Medium Value 0001H: Reference Value
50H/20H	06H/03H	0101H	EVT2 hysteresis type	0000H: Medium Value 0001H: Reference Value
50H/20H	06H/03H	0102H	EVT3 hysteresis type	0000H: Medium Value 0001H: Reference Value
50H/20H	06H/03H	0103H	EVT4 hysteresis type	0000H: Medium Value 0001H: Reference Value
50H/20H	06H/03H	0104H	EVT1 OFF side	Set value (Decimal point ignored.)
50H/20H	06H/03H	0105H	EVT2 OFF side	Set value (Decimal point ignored.)
50H/20H	06H/03H	0106H	EVT3 OFF side	Set value (Decimal point ignored.)
50H/20H	06H/03H	0107H	EVT4 OFF side	Set value (Decimal point ignored.)

(*) If 'Setting' is executed while Transmission output 2 (TA2 option) is not ordered, the following error code will be returned.

- Shinko protocol: Error code 3 (33H)
- MODBUS: Exception code 3 (03H)

Shinko Command Type	MODBUS Function Code	Data Item		Data
50H/20H	06H/03H	0108H	Number of cleansing cycles	Set value
50H/20H	06H/03H	0109H	Cleansing interval	Set value
50H/20H	06H/03H	010AH	Cleansing time	Set value
50H/20H	06H/03H	010BH	Restore time after cleansing	Set value
50H	06H	010CH	Manual cleansing mode	0001H: Manual cleansing mode
50H/20H	06H/03H	010FH	Transmission output 1 status when calibrating	0000H: Last value HOLD 0001H: Set value HOLD 0002H: Measured value
50H/20H	06H/03H	0110H	Transmission output 1 value HOLD when calibrating	Set value (Decimal point ignored.)
50H/20H	06H/03H	0111H	EVT1 pH input error alarm EVT□ type	0000H: No action 0001H: EVT2 type 0002H: EVT3 type (*1) 0003H: EVT4 type (*1)
50H/20H	06H/03H	0112H	EVT2 pH input error alarm EVT□ type	0000H: EVT1 type (*2) 0001H: No action 0002H: EVT3 type (*1) 0003H: EVT4 type (*1)
50H/20H	06H/03H	0113H	EVT3 pH input error alarm EVT□ type	0000H: EVT1 type (*2) 0001H: EVT2 type 0002H: No action 0003H: EVT4 type
50H/20H	06H/03H	0114H	EVT4 pH input error alarm EVT□ type	0000H: EVT1 type (*2) 0001H: EVT2 type 0002H: EVT3 type 0003H: No action
50H/20H	06H/03H	0115H	EVT1 pH input error alarm band when EVT□ output ON	Set value (Decimal point ignored.)
50H/20H	06H/03H	0116H	EVT1 pH input error alarm time when EVT□ output ON	Set value
50H/20H	06H/03H	0117H	EVT1 pH input error alarm band when EVT□ output OFF	Set value (Decimal point ignored.)
50H/20H	06H/03H	0118H	EVT1 pH input error alarm time when EVT□ output OFF	Set value
50H/20H	06H/03H	0119H	EVT2 pH input error alarm band when EVT□ output ON	Set value (Decimal point ignored.)
50H/20H	06H/03H	011AH	EVT2 pH input error alarm time when EVT□ output ON	Set value
50H/20H	06H/03H	011BH	EVT2 pH input error alarm band when EVT□ output OFF	Set value (Decimal point ignored.)
50H/20H	06H/03H	011CH	EVT2 pH input error alarm time when EVT□ output OFF	Set value

(*1) If 'Setting' is executed while EVT3, EVT4 outputs (EVT3 option) are/is not ordered, the following error code will be returned.

- Shinko protocol: Error code 3 (33H)
- MODBUS: Exception code 3 (03H)

(*2) If 'Setting' is executed while Transmission output 2 (TA2 option) is ordered, the following error code will be returned.

- Shinko protocol: Error code 3 (33H)
- MODBUS: Exception code 3 (03H)

Shinko Command Type	MODBUS Function Code	Data Item		Data
50H/20H	06H/03H	011DH	EVT3 pH input error alarm band when EVT□ output ON	Set value (Decimal point ignored.)
50H/20H	06H/03H	011EH	EVT3 pH input error alarm time when EVT□ output ON	Set value
50H/20H	06H/03H	011FH	EVT3 pH input error alarm band when EVT□ output OFF	Set value (Decimal point ignored.)
50H/20H	06H/03H	0120H	EVT3 pH input error alarm time when EVT□ output OFF	Set value
50H/20H	06H/03H	0121H	EVT4 pH input error alarm band when EVT□ output ON	Set value (Decimal point ignored.)
50H/20H	06H/03H	0122H	EVT4 pH input error alarm time when EVT□ output ON	Set value
50H/20H	06H/03H	0123H	EVT4 pH input error alarm band when EVT□ output OFF	Set value (Decimal point ignored.)
50H/20H	06H/03H	0124H	EVT4 pH input error alarm time when EVT□ output OFF	Set value
50H/20H	06H/03H	0125H	pH input error alarm time unit	0000H: Second(s) 0001H: Minute(s)
50H/20H	06H/03H	0126H	Transmission output 1 adjustment mode	0000H: pH/Temperature Display Mode, or Cleansing Output Mode 0001H: Transmission output 1 Zero adjustment mode 0002H: Transmission output 1 Span adjustment mode
50H/20H	06H/03H	0127H	Transmission output 1 Zero adjustment value	Set value (Decimal point ignored.)
50H/20H	06H/03H	0128H	Transmission output 1 Span adjustment value	Set value (Decimal point ignored.)
50H/20H	06H/03H	0129H	EVT1 cycle variable range	Set value (Decimal point ignored.)
50H/20H	06H/03H	012AH	EVT2 cycle variable range	Set value (Decimal point ignored.)
50H/20H	06H/03H	012BH	EVT3 cycle variable range	Set value (Decimal point ignored.)
50H/20H	06H/03H	012CH	EVT4 cycle variable range	Set value (Decimal point ignored.)
50H/20H	06H/03H	012DH	EVT1 cycle extended time	Set value
50H/20H	06H/03H	012EH	EVT2 cycle extended time	Set value
50H/20H	06H/03H	012FH	EVT3 cycle extended time	Set value
50H/20H	06H/03H	0130H	EVT4 cycle extended time	Set value
50H/20H	06H/03H	0131H	EVT1 pH fluctuation alarm time	Set value
50H/20H	06H/03H	0132H	EVT2 pH fluctuation alarm time	Set value
50H/20H	06H/03H	0133H	EVT3 pH fluctuation alarm time	Set value
50H/20H	06H/03H	0134H	EVT4 pH fluctuation alarm time	Set value
50H/20H	06H/03H	0135H	EVT1 pH fluctuation alarm band	Set value (Decimal point ignored.)
50H/20H	06H/03H	0136H	EVT2 pH fluctuation alarm band	Set value (Decimal point ignored.)
50H/20H	06H/03H	0137H	EVT3 pH fluctuation alarm band	Set value (Decimal point ignored.)
50H/20H	06H/03H	0138H	EVT4 pH fluctuation alarm band	Set value (Decimal point ignored.)

Shinko Command Type	MODBUS Function Code	Data Item		Data
50H/20H	06H/03H	0139H	EVT1 High/Low limits independent lower side value	Set value (Decimal point ignored.)
50H/20H	06H/03H	013AH	EVT2 High/Low limits independent lower side value	Set value (Decimal point ignored.)
50H/20H	06H/03H	013BH	EVT3 High/Low limits independent lower side value	Set value (Decimal point ignored.)
50H/20H	06H/03H	013CH	EVT4 High/Low limits independent lower side value	Set value (Decimal point ignored.)
50H/20H	06H/03H	013DH	EVT1 High/Low limits independent upper side value	Set value (Decimal point ignored.)
50H/20H	06H/03H	013EH	EVT2 High/Low limits independent upper side value	Set value (Decimal point ignored.)
50H/20H	06H/03H	013FH	EVT3 High/Low limits independent upper side value	Set value (Decimal point ignored.)
50H/20H	06H/03H	0140H	EVT4 High/Low limits independent upper side value	Set value (Decimal point ignored.)
50H/20H	06H/03H	0141H	EVT1 hysteresis	Set value (Decimal point ignored.)
50H/20H	06H/03H	0142H	EVT2 hysteresis	Set value (Decimal point ignored.)
50H/20H	06H/03H	0143H	EVT3 hysteresis	Set value (Decimal point ignored.)
50H/20H	06H/03H	0144H	EVT4 hysteresis	Set value (Decimal point ignored.)
50H/20H	06H/03H	0145H	Transmission output 1 status when cleansing	0000H: Last value HOLD 0001H: Set value HOLD 0002H: Measured value
50H/20H	06H/03H	0146H	Transmission output 1 value HOLD when cleansing	Set value (Decimal point ignored.)
50H/20H	06H/03H	0147H	Transmission output 2 type	0000H: pH transmission 0001H: Temperature transmission 0002H: MV2 transmission 0003H: MV3 transmission (*1) 0004H: MV4 transmission (*1)
50H/20H	06H/03H	0148H	Transmission output 2 high limit	Set value (Decimal point ignored.)
50H/20H	06H/03H	0149H	Transmission output 2 low limit	Set value (Decimal point ignored.)
50H/20H	06H/03H	014AH	Transmission output 2 adjustment mode (*2)	0000H: pH/Temperature Display Mode, or Cleaning Output Mode. 0001H: Transmission output 2 Zero adjustment mode 0002H: Transmission output 2 Span adjustment mode
50H/20H	06H/03H	014BH	Transmission output 2 Zero adjustment value	Set value (Decimal point ignored.)
50H/20H	06H/03H	014CH	Transmission output 2 Span adjustment value	Set value (Decimal point ignored.)
50H/20H	06H/03H	014DH	Transmission output 2 status when calibrating	0000H: Last value HOLD 0001H: Set value HOLD 0002H: Measured value
50H/20H	06H/03H	014EH	Transmission output 2 value HOLD when calibrating	Set value (Decimal point ignored.)

(*1) If 'Setting' is executed while EVT3, EVT4 outputs (EVT3 option) are/is not ordered, the following error code will be returned.

- Shinko protocol: Error code 3 (33H)
- MODBUS: Exception code 3 (03H)

(*2) If 'Setting' is executed while Transmission output 2 (TA2 option) is not ordered, the following error code will be returned.

- Shinko protocol: Error code 4 (34H)
- MODBUS: Exception code 17 (11H)

Shinko Command Type	MODBUS Function Code	Data Item		Data
50H/20H	06H/03H	014FH	Transmission output 2 status when cleansing	0000H: Last value HOLD 0001H: Set value HOLD 0002H: Measured value
50H/20H	06H/03H	0150H	Transmission output 2 value HOLD when cleansing	Set value (Decimal point ignored.)
50H/20H	06H/03H	0151H	pH inputs for moving average	Set value
50H/20H	06H/03H	0152H	Temperature inputs for moving average	Set value
50H/20H	06H/03H	0200H	User save area 1	-32768 to 32767 (8000H to 7FFFH)
50H/20H	06H/03H	0201H	User save area 2	-32768 to 32767 (8000H to 7FFFH)
50H/20H	06H/03H	0202H	User save area 3	-32768 to 32767 (8000H to 7FFFH)
50H/20H	06H/03H	0203H	User save area 4	-32768 to 32767 (8000H to 7FFFH)
50H/20H	06H/03H	0204H	User save area 5	-32768 to 32767 (8000H to 7FFFH)
50H/20H	06H/03H	0205H	User save area 6	-32768 to 32767 (8000H to 7FFFH)
50H/20H	06H/03H	0206H	User save area 7	-32768 to 32767 (8000H to 7FFFH)
50H/20H	06H/03H	0207H	User save area 8	-32768 to 32767 (8000H to 7FFFH)
50H/20H	06H/03H	0208H	User save area 9	-32768 to 32767 (8000H to 7FFFH)
50H/20H	06H/03H	0209H	User save area 10	-32768 to 32767 (8000H to 7FFFH)

7.4 pH Calibration, Transmission Output 1 and 2 Adjustments via Communication Command

Like a keypad operation, there are also 2 methods in pH calibration via communication command:
Automatic Calibration and Manual Calibration

7.4.1 pH Calibration

(1) Automatic Calibration Mode

The 1st standard solution [pH 7 (JIS or US standard)] selected at Data item 0009H (pH 7 calibration standard) is automatically calibrated first. Then, the 2nd standard solution [any one of pH 2, pH 4, pH 9 or pH 10 (JIS)] selected at Data item 0001H (2nd Solution) is calibrated.

pH value (based on JIS Z8802) at each temperature of pH standard solution to be calibrated is automatically calculated.

The following outlines the procedure for Automatic calibration.

• The 1st Point Automatic Calibration

- ① Immerse the pH Combined Electrode Sensor in the 1st standard solution (pH 7).
When selecting Last value HOLD (0000H) at Data item 010FH (Transmission output 1 status when calibrating) or at 014DH (Transmission output 2 status when calibrating), select it while the pH Combined Electrode Sensor is being immersed in the solution currently calibrated.
After that, immerse the pH Combined Electrode Sensor in the 1st point standard solution (pH 7).
- ② Set Data item 0038H (pH calibration mode) to 0001H.
The unit proceeds to pH calibration mode.
- ③ Set Data item 0039H (pH calibration start) to 0001H.
The 1st Point Automatic Calibration starts.
- ④ If 2^{13} , 2^{12} digits are read at Data item 0081H (Status flag 1), 01 (During the 1st point calibration) will be returned during automatic calibration.
Automatic Calibration is performed using the Automatic electrode quality evaluation function.
- ⑤ If 2^{13} , 2^{12} digits are read at Data item 0081H (Status flag 1), 00 (Standby) will be returned after automatic calibration is completed.
- ⑥ Set 0039H (pH calibration start) to 0002H.
The 1st point Automatic Calibration is complete, and the unit moves to the 2nd point Automatic Calibration mode.

• The 2nd Point Automatic Calibration

- ① After the electrode is rinsed, immerse the pH Combined Electrode Sensor in the 2nd standard solution.
- ② Set the Data item 0039H (pH calibration start) to 0003H.
Automatic calibration for the 2nd point starts.
- ③ If 2^{13} , 2^{12} digits are read at Data item 0081H (Status flag 1), 10 (During the 2nd point calibration) will be returned during automatic calibration.
Automatic calibration is performed using the Automatic electrode quality evaluation function.
- ④ If 2^{13} , 2^{12} digits are read at Data item 0081H (Status flag 1), 11 (Calibration complete) will be returned after automatic calibration is completed.
- ⑤ Set Data item 0039H (pH calibration start) to 0004H.
Automatic calibration for the 2nd point is complete.
- ⑥ Set Data item 0038H (pH calibration mode) to 0000H.
The pH automatic calibration is complete, and the unit reverts to pH/Temperature Display Mode, or Cleansing Output Mode.

(2) Manual Calibration Mode

When there is a difference of pH 2 or more, Manual calibration can be performed using the randomly selected 2 kinds of solution.

The following outlines the procedure for Manual calibration.

• The 1st Point Manual Calibration

- ① Immerse the pH Combined Electrode Sensor in the 1st standard solution.
When selecting Last value HOLD (0000H) at Data item 010FH (Transmission output 1 status when calibrating) or at 014DH (Transmission output 2 status when calibrating), select it while the pH Combined Electrode Sensor is being immersed in the solution currently calibrated.
After that, immerse the pH Combined Electrode Sensor in the 1st point standard solution.
- ② Set Data item 0038H (pH calibration mode) to 0001H.
- ③ Set Data item 0039H (pH calibration start) to 0001H.
Manual calibration for the 1st point starts.
- ④ If 2^{13} , 2^{12} digits are read at Data item 0081H (Status flag 1), 01 (During the 1st point calibration) will be returned during manual calibration.
- ⑤ Set a pH calibration value at Data item 0008H (pH calibration value).
- ⑥ Set Data item 0039H (pH calibration start) to 0002H.
Manual calibration for the 1st point is complete, and the unit enters the 2nd point Manual calibration mode.
- ⑦ If 2^{13} , 2^{12} digits are read at Data item 0081H (Status flag 1), 00 (Standby) will be returned after manual calibration is complete.

• The 2nd Point Manual Calibration

- ① Rinse the electrode, then immerse the pH Combined Electrode Sensor in the 2nd standard solution.
- ② Set Data item 0039H (pH calibration start) to 0003H.
Manual calibration for the 2nd point starts.
- ③ If 2^{13} , 2^{12} digits are read at Data item 0081H (Status flag 1), 10 (During the 2nd point calibration) will be returned during manual calibration.
- ④ Set a pH calibration value at Data item 0008H (pH calibration value).
- ⑤ Set Data item 0039H (pH calibration start) to 0004H.
Manual calibration for the 2nd point is complete.
- ⑥ If 2^{13} , 2^{12} digits are read at Data item 0081H (Status flag 1), 11 (Calibration complete) will be returned after manual calibration is complete.
- ⑦ Set Data item 0038H (pH calibration mode) to 0000H.
The pH manual calibration is complete, and the unit reverts to pH/Temperature Display Mode, or Cleansing Output Mode.

(3) Error Code during pH Calibration

If pH Calibration cannot be performed due to unstable pH input, temperature compensation error, etc., the "Error code 1 (Error, Burnout, Short-circuited, etc.)" will be returned after 2^0 to 2^{10} digits are read at Data item 0081H (Status flag 1).

To release the Error code, set Data item 0038H (pH calibration mode) to 0000H.

The unit returns to pH/Temperature Display Mode, or Cleansing Output Mode.

If Data item 0039H (pH calibration start) is set during pH calibration of the 1st or 2nd point, the following error code will be returned:

Shinko protocol: Error code 34H

MODBUS protocol: Exception code 11H

7.4.2 Transmission Output 1 Adjustment

Fine adjustment of Transmission output 1 is performed.

This pH meter is adjusted at the factory, however, differences may occur between the indication value of the connected equipment (recorders, etc.) and the output value of this instrument.

In this case, perform Transmission output 1 Zero adjustment and Span adjustment.

The following outlines Transmission output 1 adjustment procedure.

- ① Set Data item 0126H (Transmission output 1 adjustment mode) to 0001H.
The unit moves to Transmission output 1 Zero adjustment mode.
If 2¹², 2¹¹ digits are read at Data item 0091H (Status flag 2), 01 (During Transmission output 1 Zero adjustment in Transmission output 1 adjustment mode) will be returned.
- ② Set the Transmission output 1 Zero adjustment value at Data item 0127H (Transmission output 1 Zero adjustment value), while viewing the value indicated on the connected equipment (recorders, etc.).
Setting range: $\pm 5.00\%$ of Transmission output 1 span
- ③ Set Data item 0126H (Transmission output 1 adjustment mode) to 0002H.
The unit moves to Transmission output 1 Span adjustment mode.
If 2¹², 2¹¹ digits are read at Data item 0091H (Status flag 2), 10 (During Transmission output 1 Span adjustment in Transmission output 1 adjustment mode) will be returned.
- ④ Set Transmission output 1 Span adjustment value at Data item 0128H (Transmission output 1 Span adjustment value), while viewing the value indicated on the connected equipment (recorders, etc.).
Setting range: $\pm 5.00\%$ of Transmission output 1 span
- ⑤ Repeat steps ① to ④ if necessary.
- ⑥ To finish the Transmission output 1 adjustment, set Data item 0126H (Transmission output 1 adjustment mode) to 0000H.
The unit reverts to pH/Temperature Display Mode, or Cleansing Output Mode.

7.4.3 Transmission Output 2 Adjustment

Fine adjustment of Transmission output 2 is performed.

This pH meter is adjusted at the factory, however, differences may occur between the indication value of the connected equipment (recorders, etc.) and the output value of this instrument.

In this case, perform Transmission output 2 Zero adjustment and Span adjustment.

The following outlines Transmission output 2 adjustment procedure.

- ① Set Data item 014AH (Transmission output 2 adjustment mode) to 0001H.
The unit moves to Transmission output 2 Zero adjustment mode.
If 2¹⁴, 2¹³ digits are read at Data item 0091H (Status flag 2), 01 (During Transmission output 2 Zero adjustment in Transmission output 2 adjustment mode) will be returned.
- ② Set the Transmission output 2 Zero adjustment value at Data item 014BH (Transmission output 2 Zero adjustment value), while viewing the value indicated on the connected equipment (recorders, etc.).
Setting range: $\pm 5.00\%$ of Transmission output 2 span
- ③ Set Data item 014AH (Transmission output 2 adjustment mode) to 0002H.
The unit moves to Transmission output 2 Span adjustment mode.
If 2¹⁴, 2¹³ digits are read at Data item 0091H (Status flag 2), 10 (During Transmission output 2 Span adjustment in Transmission output 2 adjustment mode) will be returned.
- ④ Set Transmission output 2 Span adjustment value at Data item 014CH (Transmission output 2 Span adjustment value), while viewing the value indicated on the connected equipment (recorders, etc.).
Setting range: $\pm 5.00\%$ of Transmission output 2 span
- ⑤ Repeat steps ① to ④ if necessary.
- ⑥ To finish the Transmission output 2 adjustment, set Data item 014AH (Transmission output 2 adjustment mode) to 0000H.
The unit reverts to pH/Temperature Display Mode, or Cleansing Output Mode.

7.5 Notes on Programming Monitoring Software

7.5.1 How to speed up the scan time

When monitoring multiple units of AER-102-PH, set the program so that the requisite minimum pieces of data such as Data item 0080H (pH), Data item 0090H (Temperature), Data item 0081H (Status flag 1), Data item 0091H (Status flag 2) can be read. For other data, set the program so that they can be read only when their set value has been changed. This will speed up the scan time.

7.5.2 How to read the set value changes made by the front keypad operation

If any set value is changed by keypad operation, the AER-102-PH will set [0081H (Status flag 1) 2¹⁵: Change in key operation] to 1 (Yes).

There are 2 methods of reading the set value changes made by the front keypad.

(1) Reading method 1

- ① On the monitoring software side, check that [0081H (Status flag 1) 2¹⁵: Change in key operation] has been set to 1 (Yes), then read all set values.
- ② Clear the [0081H (Status flag 1) 2¹⁵: Change in key operation], by setting [Data item 007FH (Key operation change flag clearing)] to [Clear change flag (0001H)].
If [007FH (Key operation change flag clearing)] is set to [Clear change flag (0001H)] during setting mode of the instrument, Error code 5 (35H, Shinko protocol) or Exception Code 18 (12H, MODBUS protocol) will be returned as a negative acknowledgement. And [0081H (Status flag 1) 2¹⁵: Change in key operation] cannot be cleared.
Set a program so that all set values can be read when a negative acknowledgement is returned.
- ③ Read all set values again after acknowledgement is returned.

(2) Reading method 2

- ① On the monitoring software side, check that [0081H (Status flag 1) 2¹⁵: Change in key operation] has been set to 1 (Yes), then set 007FH (Key operation change flag clearing) to 0001H (Clear change flag).
- ② Set the program depending on acknowledgement or negative acknowledgement as follows.
When acknowledgement is returned:
Consider it as settings completed, and read all set values.
When Error code 5 (35H, Shinko protocol) or Exception code 18 (12H, MODBUS protocol) is returned as a negative acknowledgement:
Consider it as still in setting mode, and read the requisite minimum pieces of data such as 0080H (pH), 0090H (Temperature), 0081H (Status flag 1), 0091H (Status flag 2), then return to step ①.

Thus, programs which do not affect the scan time can be created using the methods described above, even if set values on the monitoring software will not be updated until settings are complete.

7.5.3 Note when sending all set values at one time

- If EVT1, EVT2, EVT3 or EVT4 type is changed at Data items 0003H (EVT1 type), 0050H (EVT2 type), 0051H (EVT3 type) or 0052H (EVT4 type), the EVT1, EVT2, EVT3 or EVT4 value will default to 0 (zero). The output status of EVT1, EVT2, EVT3 or EVT4 will also be initialized.

First, send the EVT1, EVT2, EVT3, EVT4 type, then send the EVT1, EVT2, EVT3, EVT4 value set at Data items 0004H (EVT1 value), 0053H (EVT2 value), 0054H (EVT3 value) and 0055H (EVT4 value).

8. Specifications

Serial communication	The following operations can be carried out from an external computer. (1) Reading and setting of various set values (2) Reading of the pH, temperature and status (3) Function change, adjustment (4) Reading and setting of user save area			
Cable length	1.2 km (Max.), Cable resistance: Within 50 Ω (Terminators are not necessary, but if used, use 120 Ω minimum on one side.)			
Communication line	EIA RS-485			
Communication method	Half-duplex communication			
Communication speed	9600, 19200, 38400 bps (Selectable by keypad)			
Synchronization	Start-stop synchronization			
Code form	ASCII, Binary			
Communication protocol	Shinko protocol, MODBUS ASCII, MODBUS RTU (Selectable by keypad)			
Data bit/Parity	8 bits/No parity, 7 bits/No parity, 8 bits/Even, 7 bits/Even, 8 bits/Odd, 7 bits/Odd (Selectable by keypad)			
Stop bit	1 bit, 2 bits (Selectable by keypad)			
Error correction	Command request repeat system			
Error detection	Parity check Checksum (Shinko protocol) LRC (MODBUS protocol ASCII) CRC-16 (MODBUS protocol RTU)			
Data format	Communication Protocol	Shinko Protocol	MODBUS ASCII	MODBUS RTU
	Start bit	1	1	1
	Data bit	7	7 (8) Selectable	8
	Parity	Even	Even, (No parity Odd) Selectable	No parity (Even, Odd) Selectable
	Stop bit	1	1 (2) Selectable	1 (2) Selectable

9. Troubleshooting

Check that power is being supplied to the master and slave that customers use. If communication failure still occurs, check the following.

Problem	Possible Cause	Solution
Communication failure	Communication cable is not securely connected, or is disconnected/ defective.	Make sure that the communication connector is securely connected.
	Incorrect wiring of the communication cable and/or connector	Check the communication cable and connector.
	Imperfect contact between the communication cable and the connector, or between the communication connector and instrument port	Check the communication cable and the connector.
	Communication speed of the slave does not match that of the master.	Check the communication speed of the slave and master.
	The data bit, parity and stop bit of the master do not correspond to those of the slave.	Check the data bit, parity and stop bit of the master and the slave.
	The instrument number (address) of the slave does not correspond to that of the command.	Check the instrument number (address) of the slave and command.
	The instrument numbers (addresses) are duplicated in multiple slaves.	Check the instrument numbers (addresses) of the slave.
	Make sure that the program is appropriate for the transmission timing.	Check the program.
Although communication is occurring, the response is negative acknowledgement.	A non-existent command code has been sent.	Check the command code.
	The setting command data exceeds the setting range of the slave.	Check the setting range.
	The AER-102-PH cannot be set while calibration is being performed using the Automatic electrode quality evaluation function.	Check the slave status.
	The AER-102-PH is in the front keypad operation setting mode.	Return the unit to pH/Temperature Display Mode, or Cleansing Output Mode.

For all other malfunctions, please contact our main office or dealers.

SHINKO TECHNOS CO., LTD.
OVERSEAS DIVISION

Head Office : 2-5-1, Senbahigashi, Minoo, Osaka, Japan

URL: <http://www.shinko-technos.co.jp/e/>

E-mail: overseas@shinko-technos.co.jp

Tel : +81-72-727-6100

Fax: +81-72-727-7006